

COMPUTER SIMULATION OF CARDIAC ELECTRICAL ACTIVITY USING AN ELECTROCARDIOGRAPHON NANOSENSORS

M. G. Grigor'yev, N. V. Turushev

Medical Instrument-Making lab №63, Institute of Non-Destructive Testing, National Research Tomsk Polytechnic University, 30, Lenin av., Tomsk, 634050, Russia
E-mail: Mishatpu@mail.ru

The issues related to cardiovascular diseases are considered. The method to solve some of the existing problems has been proposed. Also a two-component Aliev-Panfilov model and the algorithm of the hardware- software complexes are discussed. The obtained results are presented.

Keywords:

Functional diagnostic, electrocardiographic, cardiovascular system, transmembrane potential.

Introduction

According to World Health Organization (WHO), over 17 million people worldwide die annually from cardiovascular diseases (CVDs). Moreover, according to WHO, an estimated number of almost 23.6 million people will die from CVDs by 2030. In 2012, 1 million 232 thousand 182 people died from CVDs in Russia (Fig.1) [1, 2, 3, 4, 5].

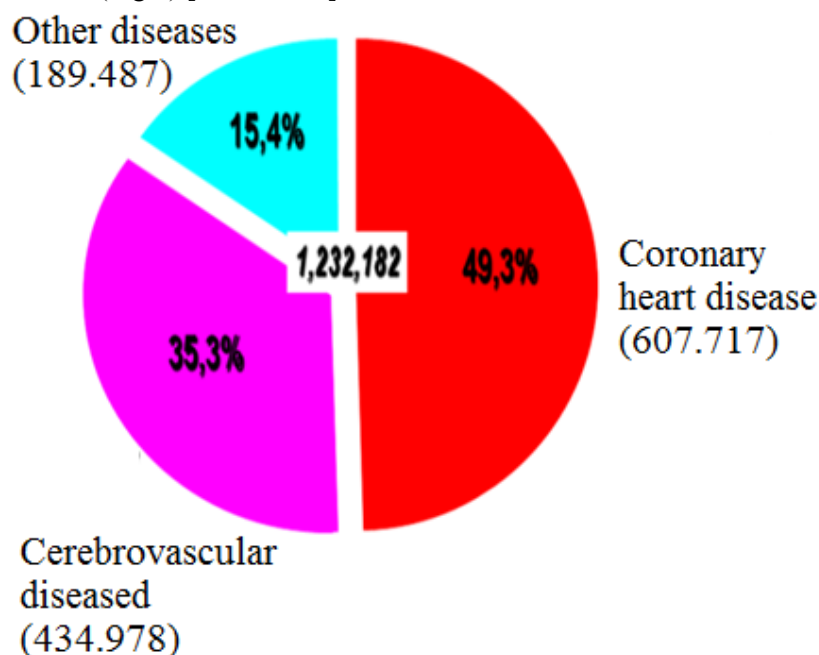


Fig. 1. WHO report on CVDs for 2012

Electrocardiographic (ECG) method is a most common method to examine the state of a patient's cardiovascular system in various medical institutions. ECG is referred to as the method of functional diagnostics with a quantitative evaluation of the research results. The first cardiographic research was carried out by the Scottish scientist Alexander Muirhead in the late 19th century [6, 7].

Analysis of manufactures

A body is known to be a 3-D conductor. The cardiac activity results in electromagnetic field generation, which can be measured from the body surface. The field is constantly changing under heart excitation and characteristics of the field depend on the moving direction of the excitation wave

passing through the heart. The analysis of the electromagnetic field allows us to consider the sequence of atrial and ventricular excitation.

Lots of companies are trying to solve this problem, but just some of them managed to succeed. The analysis proved the absence of the hardware and software complexes for mass application (in departments of functional diagnostics and cardiology, in hospitals and clinics, in ambulances, as well as in private medical practice, and at home) to be used in a non-invasive detailed study of the heart by registering low-amplitude potentials of the heart from the surface of the human body without filters and cardiac cycle averaging. Such devices are presented in Table 1.

Table 1. Overview of the manufactures [8, 9, 10, 11].

Company name	Number electrode placing points	Signal Level, μV	Frequency range, Hz	Cost
Geolink-electronics (Russia)	3	6	0,03-10,0	\$7700
Rozinn (USA)	3	8	0.05-70	\$11000
OXFORD (England)	3	5	0,05-100	\$11400
NRTPU (Russia)	3-12	0,3	0-10000	<\$1400
Davis Medical Electronics Inc. (USA)	3-12	2	0.05-60	\$6500
HELLIGE (USA)	3-12	5	0,05 -100	\$12000
CardioMem CM 3000 (Germany)	3	8	0,03-70	\$4600
Scan Tech Medical, LLC (USA)	3	6	0.05-100	\$4700

The Table shows that the commercial value of cardiographs by known companies are excessively large compared to the product suggested. This is due to the fact that the nanosensors developed for this device make possible to receive signals of a nanovolt level without filters and cardiac cycle averaging.

Heart electricity activity

The development of a new generation of nanosensors and computerized ECG – the apparatus of high resolution to be used in clinics and at home – is relevant for improving the diagnostics of cardiovascular diseases, including early heart diagnostics of adults, children, infants and the fetus.

To solve the problem, a numerical model of excitation propagation in the heart muscle is to be studied.

Excitation propagates through the heart tissue at a certain rate, varies for different parts of the heart (Fig. 2).

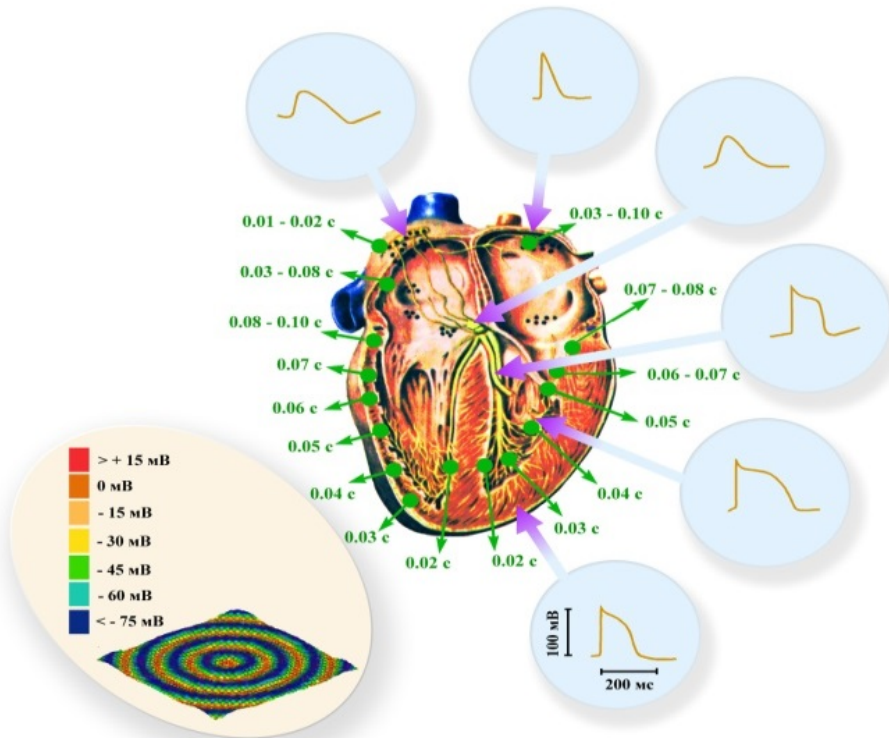


Fig. 2. Space-time scheme of a regular cardiac work of a human being

Green lettering and arrows indicate the time of the excitation wave arrival at this region of the heart. Blue insets show the shape of the traveling-wave profile (the so-called "action potential") in different regions of the heart due to difference in properties of the excitable medium formed by the heart tissue. The beige inset demonstrates regular propagation of the traveling-wave excitation from the pacemaker area in the center (sinus node) towards the edges (along the working myocardium) in the simplest mathematical simulation model [12].

This results in a space-time scheme of heart excitation which ensures its functioning. In modeling excitation propagation, all the features of heart excitation are to be considered.

Mathematical simulation

To simulate excitation propagation, one of the simplest models of the excitable medium, a two-component Aliev-Panfilov model is suggested in [13, 14]. The model is implemented in the form of "reaction-diffusion" equations.

$$\frac{\partial u}{\partial t} = -ku \cdot (u - a) \cdot (u - 1) - uv + \Delta u, \quad (1)$$

$$\frac{\partial v}{\partial t} = - \left(\varepsilon_0 + \frac{\mu_1 v}{u + \mu_2} \right) \cdot (v + ku \cdot (u - a - 1)), \quad (2)$$

where (1) $u(x, y, t)$ is a dimensionless function, corresponding to the transmembrane potential, and (2) $v(x, y, t)$ is a dimensionless function corresponding to a slow membrane recovery current. The bonds between the heart muscle cells are defined by diffusion terms of the equations, and the dynamics of a single cell is defined by nonlinear terms of the equations. After a series of experiments [15], for better concordance of the system to the properties of the heart muscle the model parameters were determined: $k = 8.0$, $\varepsilon_0 = 0.01$, $\mu_1 = 0.2$, $\mu_2 = 0.3$, $a = 0.15$.

Hardware-software complex as a solution

To implement the simulation of the excitation propagation in the heart within the concept of the cardiovascular system (CVS) assessment a hardware-software complex (HSC) is going to be developed in Laboratory No 63, Institute of Non-Destructive Testing. The algorithm of its functioning is shown in Figure 3.

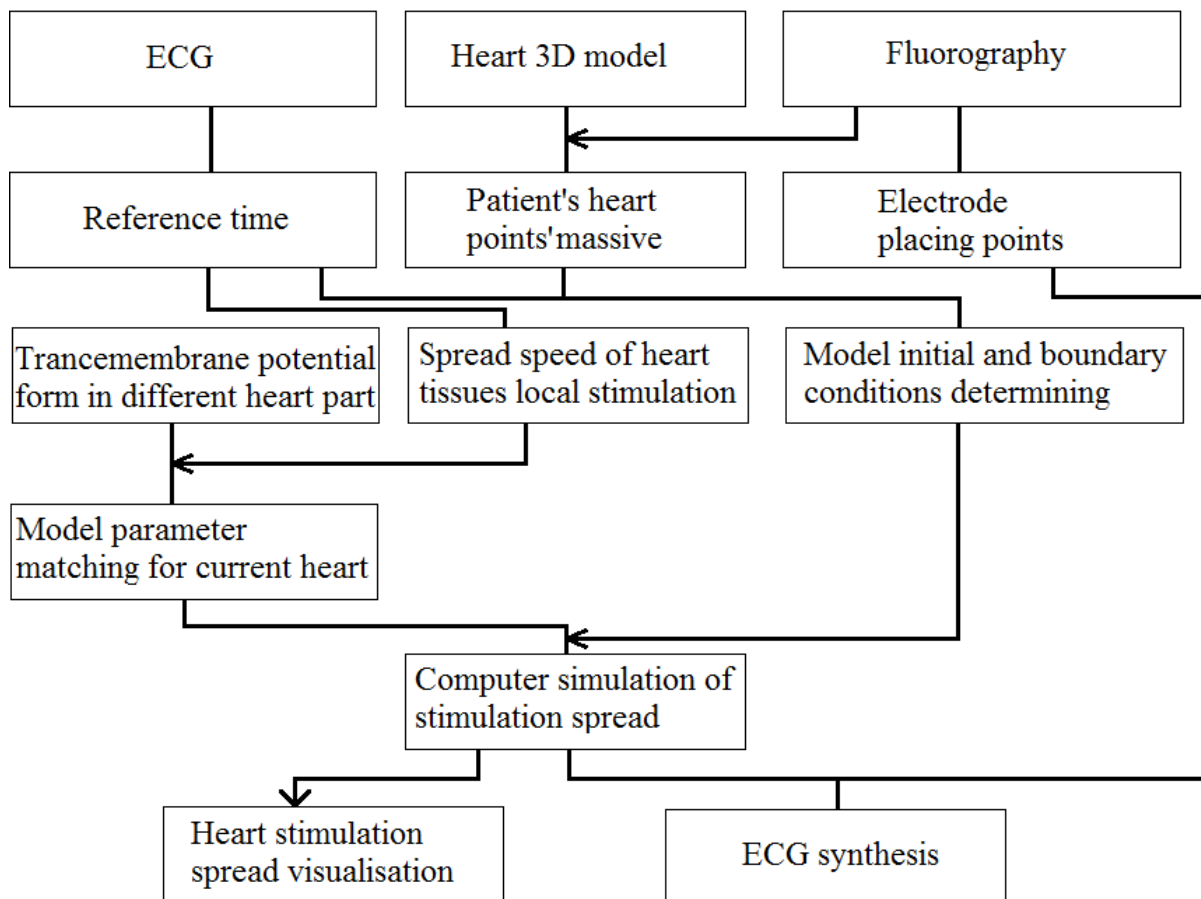


Fig. 3. The algorithm for simulation of excitation propagation in the heart.

According to the algorithm, at first, the initial and boundary conditions of the model are assigned basing on the cardiographic information analysis. After that, the model parameters are determined for various compartments of the heart, and the excitation propagation is simulated. The simulation results are used to visualize excitation propagation on the heart surface.

Conclusion

The model of the cardiac electrical activity makes possible to determine the "electrical portrait" of the patient's heart within the cardiac cycle, which enables to identify the diagnostic features in the analysis of indirect parameters determined by simulating the electrical processes in the heart and ECG output data from nanosensors.

REFERENCES

1. Baranov V. A., Avdeeva D. K., Grigoriev M. G. Grigoriev, Structural approach to inverse problems of computerized diagnostics in cardiology // Modern problems of science and education. – 2013. - № 6. – URL: <http://www.science-education.ru/113-11343>
2. D. K. Avdeeva, O. N. Vylegzhanin, Extraction from registered cardioimpulse orthogonal to it low-amplitude component // Naukovedenie. – 2013. - № 6. – URL: <http://naukovedenie.ru/PDF/153TVN613.pdf>

3. D. K. Avdeeva, V. Yu. Kazakov, N. M. Natalinova, M. L. Ivanov, The results modeling of high frequency filter and low-pass filter effects to the micropotentials recording quality on the electrocardiogram // *Naukovedenie*. – 2013. - № 6. – URL: <http://naukovedenie.ru/PDF/154TVN613.pdf>
4. D. K. Avdeeva, N. V. Turushev, N. M. Natalinova, M. L. Ivanov, Analysis of the impact of filtering links on electroencephalogram and electromyogram registered channel highly sensitive to nanoelectrodes. // *Naukovedenie*. – 2013. - № 6. – URL: <http://naukovedenie.ru/PDF/155TVN613.pdf>
5. Data and statistics. – URL: <http://www.who.int/research/en/> (Date of access: 24.04.2014).
6. Alexander Muirhead. – URL: http://en.wikipedia.org/wiki/Alexander_Muirhead (Date of access: 25.04.2014).
7. Medgroup holding. – URL: <http://www.med-group.ru/manufacture/15/> (Date of access: 25.04.2014).
8. University of oxford. – URL: <http://www.ox.ac.uk/> (Date of access: 25.04.2014).
9. Davis medical electronics. – URL: <http://www.davismedical.com/> (Date of access: 25.04.2014).
10. GE Healthcare. – URL: <http://www3.gehealthcare.co.uk/en-GB/Products> (Date of access: 25.04.2014).
11. Basic Mechanisms of Cardiac Arrhythmias. – URL: <http://www.intechopen.com/books/cardiac-arrhythmias-mechanisms-pathophysiology-and-treatment/basic-mechanisms-of-cardiac-arrhythmias> (Date of access: 26.04.2014).
12. O. N. Bodin, A. V. Kuz'min, A. N. Mitroshin, Development of visual models of heart for learning medical students // *University proceedings. Volga region. Medical sciences*. – 2007. - № 2. – URL: <http://cyberleninka.ru/article/n/razrabotka-vizualnoy-modeli-serdtsa-dlya-obucheniya-studentov-medikov>
13. Mathematical cell. – URL: http://www.mathcell.ru/ru/obzors/obzor_Elkin2.shtml (Date of access: 26.04.2014).
14. Aliev R., Panfilov A. A simple two-variable model of cardiac excitation // *Chaos, Solutions & Fractals*. – 1996. - № 7. – pp. 293–301.

Authors' information:

Grigor'yev M. G.: Tomsk, graduate student of Institute of Non-Destructive Testing, National Research Tomsk Polytechnic University

Turushev N. V.: Tomsk, graduate student of Institute of Non-Destructive Testing, National Research Tomsk Polytechnic University